



Project 438

Instrument:	2250-L
Application:	BZ7132 Version 3.1
Start Time:	08/27/2013 11:22:02
End Time:	08/27/2013 11:22:35
Elapsed Time:	00:00:33
Bandwidth:	1/3-octave
Max Input Level:	142.02


	Time	Frequency
Broadband (excl. Peak):	FSI	AC
Broadband Peak:		C
Spectrum:	FS	A

Instrument Serial Number:	2701788
Microphone Serial Number:	2678792
Input:	
Windscreen Correction:	None
Sound Field Correction:	Free-field

Calibration Time:	12/04/2012 08:41:08
Calibration Type:	External reference
Sensitivity:	44.1560298204422 mV/Pa

Project 438

	Start time	End time	Elapsed time	Overload [%]	LAeq [dB]	LAFmax [dB]	LAFmin [dB]
Value				0.00	61.5	63.7	59.1
Time	11:22:02	11:22:35	0:00:33				
Date	27/08/2013	27/08/2013					

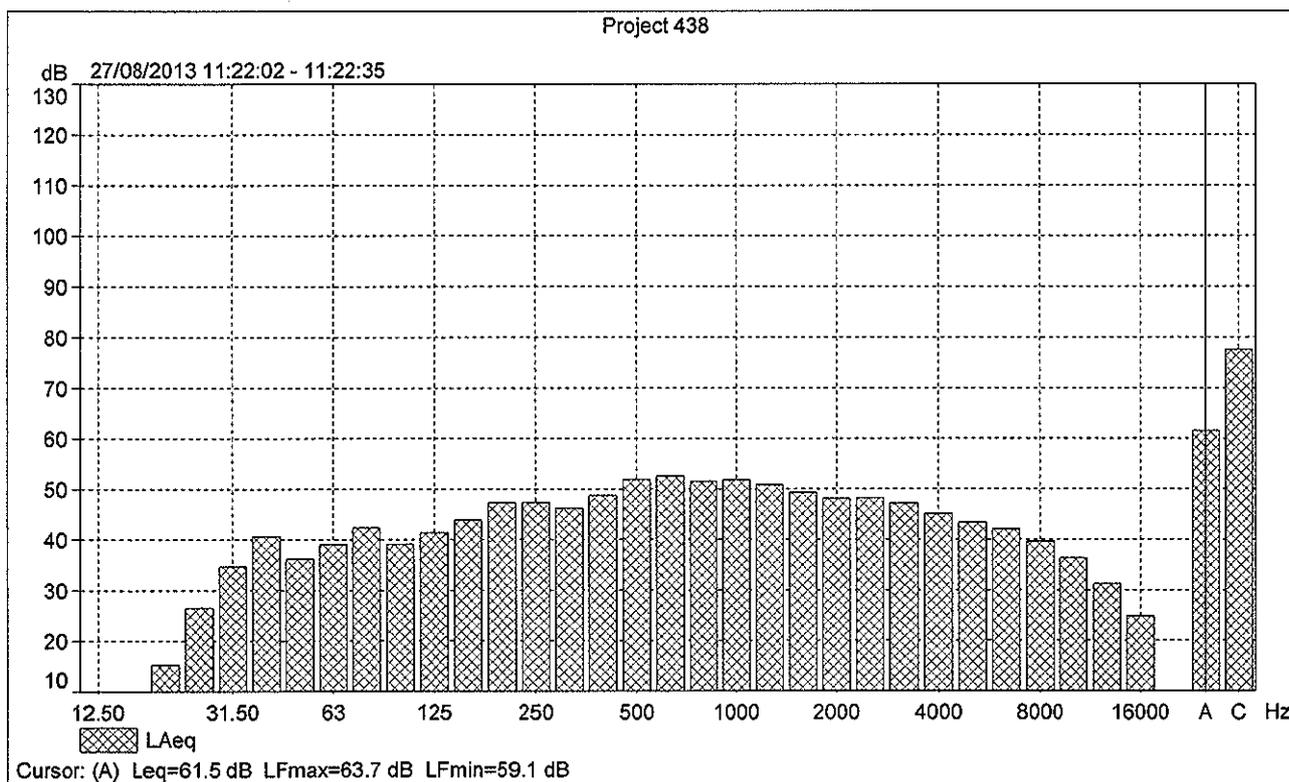



Project 438

